


# Ghost-Guard-LC - Column Certificate


## Column Data:

Batch No. E02031  
 Art.-No. ANP00001  
 Art. Ghost-Guard-LC (ID 4.6, L 30 mm)  
 Packaging Material C05001

## Chromatogram without using the Ghost-Guard-LC:

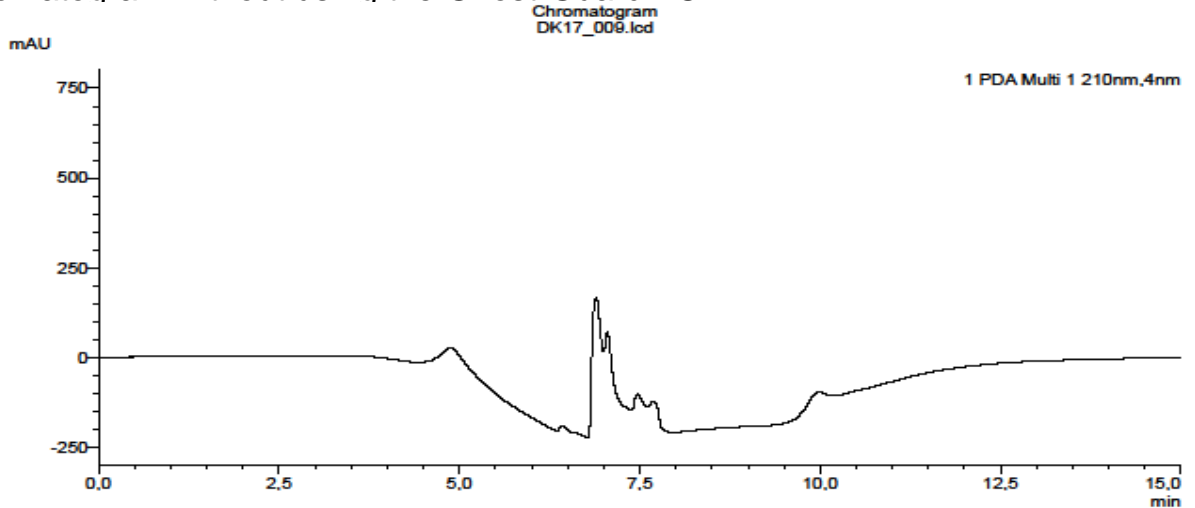

## Chromatogram using the Ghost-Guard-LC:

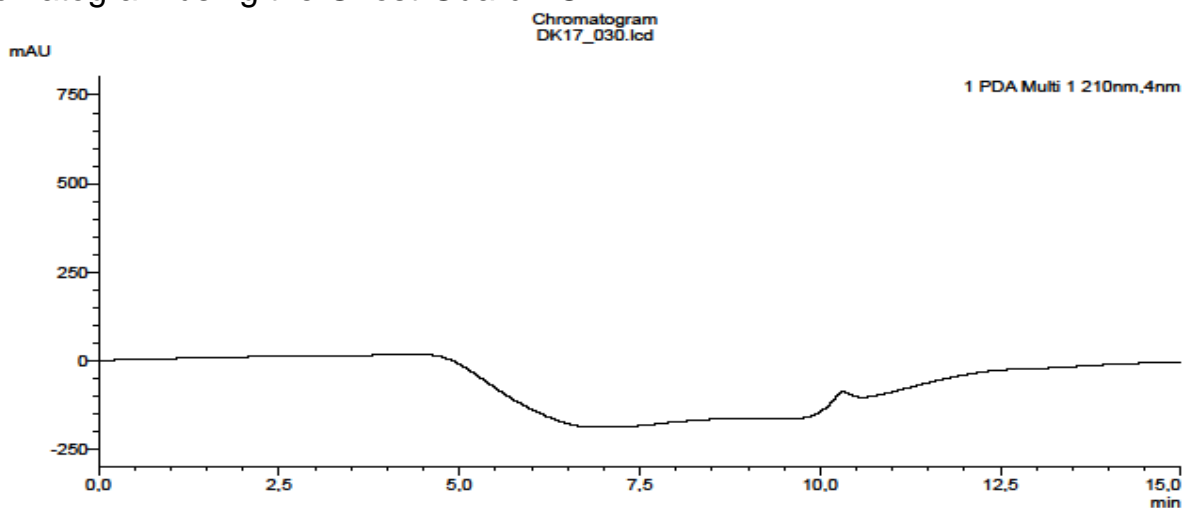

## Chromatographic Test Conditions:

Analytical Column Omnyx monolytic-C18, 50x4.6mm  
 Detection UV 210 nm  
 Injection No injection (blank run)  
 Mobile Phase A 10 mM ammonium acetate in water  
 Mobile Phase B Methanol  
 Gradient

Min	% A	% B	% C	ml/Min
0.0	95	5	-	1
1.0	95	5	-	1
4.0	5	95	-	1
7.0	5	95	-	1
7.5	95	5	-	1
15.0	95	5	-	1