





## OLIGONUCLEOTIDES

### INTRODUCTION


The application shows the purification of nucleotides on ARION® column compared with our competitors' BDS and BDS-clone columns.

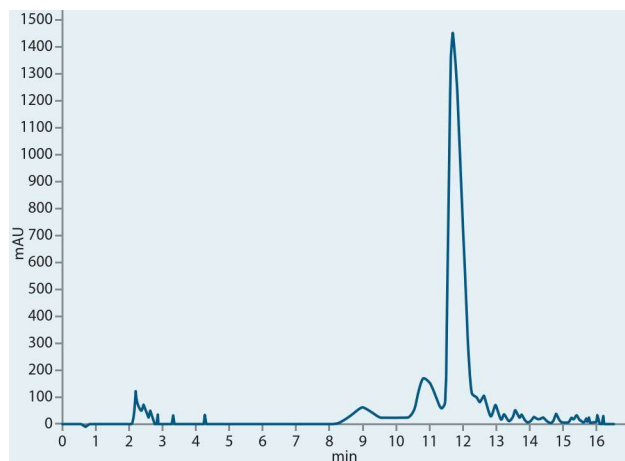


HEX BHQ probe on ARION® (DAD)

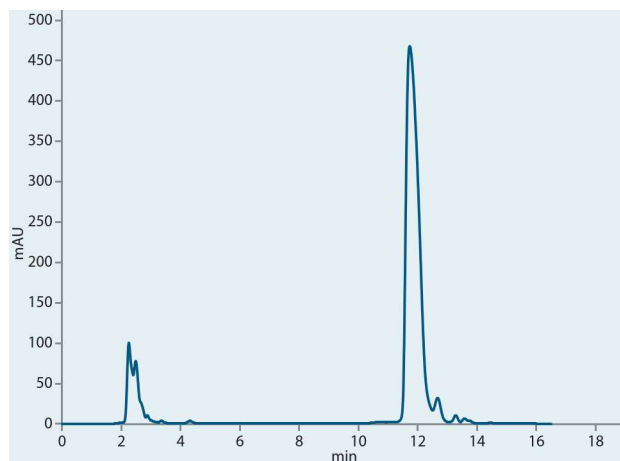

HEX BHQ probe on ARION® (FLD)

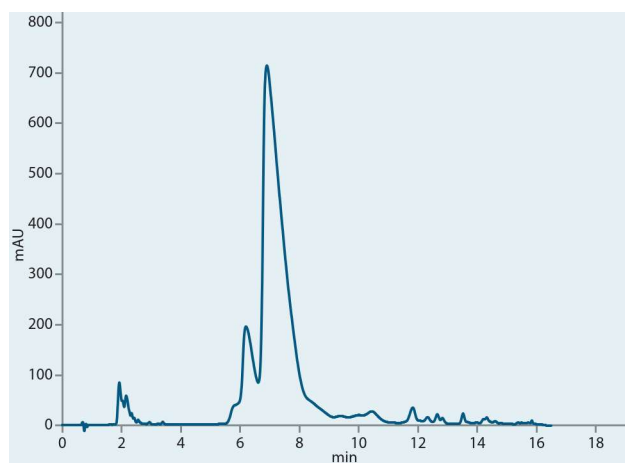


HEX BHQ probe on BDS column (DAD)

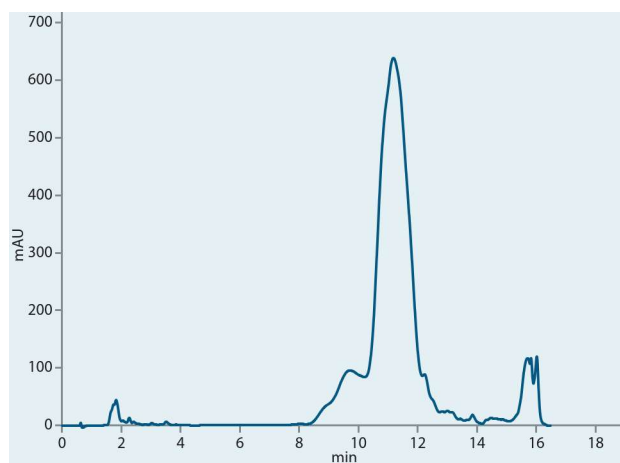

HEX BHQ probe on BDS-clone column (DAD)

<b>Column</b>	ARION® Plus C18, 5.0 µm
<b>Dimensions</b>	100 mm × 4.6 mm
<b>Part number</b>	ARI-5720-LI46
<b>Mobile Phase</b>	(A) 50mM TEAA (B) MeOH : Acetonitrile (1 : 1v/v), gradient elution
<b>Flow rate</b>	Proprietary
<b>Injection</b>	50 µl
<b>Temperature</b>	Ambient
<b>Detection</b>	DAD, FLD @534 nm (Ex), 556 nm (Em)



AUTHORIZED DISTRIBUTOR

MZ-Analysentechnik GmbH  
 Barcelona-Allee 17 • D-55129 Mainz  
 Tel +49 6131 880 96-0  
 Fax +49 6131 880 96-20  
 e-mail: info@mz-at.de  
 www.mz-at.de