

Features

Coregel columns are packed with chemically resistant polymeric polystyrene divinylbenzene copolymers varying in percent cross-linkage and particle sizes. Coregel columns provide the following benefits compared to silica based columns:

- Stable in the pH range of 0 to 14
- Stable at high temperatures up to 90 °C
- Consistent performance through numerous sample injections (depending on sample preparation, instrument maintenance, and the use of guard systems)
- No need for gradients for sample analysis due to the use of simple dilute acid — allowing the use of universal detectors such as refractive index (RI) detectors
- Eliminates the need for high cost solvents (including waste disposal)
- Eluent serves as a self-regenerating cleaning solution and does not degrade the column

The chart below is a general guideline for choosing your Concise Separations column:

RESOLUTION (HIGHEST TO LOWEST)	ANALYSIS TIME (FASTER TO SLOWER)	SELECTIVITY (HIGHER TO LOWER)	DURABILITY (MORE TO LESS)
Coregel ION 300	Coregel USP L17	Coregel ION 300	Coregel 107H
Coregel 64H	Coregel 87H1	Coregel 64H	Coregel 87H3
Coregel WA1	Coregel ION 310	Coregel ORH 801	Coregel 87H1
Coregel 87H3	Coregel ARH 601	Coregel WA1	Coregel WA1
Coregel ORH 801	Coregel ORH 801	Coregel 87H3	Coregel ORH 801
Coregel 107H	Coregel 107H	Coregel 107H	Coregel ION 310
Coregel ARH 601	Coregel 87H3	Coregel ARH 601	Coregel USP L17
Coregel ION 310	Coregel WA1	Coregel ION 310	Coregel ARH 601
Coregel 87H1	Coregel 64H	Coregel 87H1	Coregel 64H
Coregel USP L17	Coregel ION 300	Coregel USP L17	Coregel ION 300

How to Choose a Column for Your Sample

In choosing the best column for your application, there are several factors to consider:

- Resolution of peaks of interest
- Analysis time
- Selectivity (elution order of peaks)
- Durability

In general, the **Coregel 87H3** is a good starting point when considering a Concise Separations organic acids analysis column since it combines good resolution of many common organic acids, with high durability. However, the many combinations of polymer cross-linkage, particle size and column sizes offered by Concise Separations allow customers to choose a column with features most important to maximize their separation needs.

Another valuable tool for selecting a column is to use retention charts of many common organic acids. Due to the abundance of organic acids, sugars, and alcohols, and the innumerable possible combinations of the compounds in mixtures, it is impossible to have a totally comprehensive retention chart to conclusively guide a chemist through all applications. Since we stock most of the common organic acids, sugars and alcohols in our laboratory, we frequently will generate a sample chromatogram of your particular sample mixture, or will actually run your sample to ensure that our columns will separate your sample. Please contact Concise Separations for any questions regarding column selection.

Concise Separations Offers More Column Options

Concise Separations has a wider variety of polymeric HPLC columns than our competitors. The vast majority of columns on the market for ion-exclusion analysis of organic acids utilize an 8% cross-linked polystyrene divinylbenzene copolymer.

Although the 8% cross-linked polymeric columns provide an excellent separation of many typical samples containing organic acids, sugars and alcohols, Concise Separations has determined that by varying the cross-linkage and particle sizes of the polymers, certain separations are enhanced tremendously. Although ion-exclusion of organic acids is the main separation mechanism for samples, the size exclusion limit of the polymers is controlled by the percent cross-

linking. The additional size exclusion mechanism for Concise Separations columns provide unique selectivity for some components. For maximum efficiency, Concise Separations also provides columns with smaller particle sizes and tighter size distributions than the typical industry standard of 9 micron particles. By providing additional choices, Concise Separations allows you to maximize separations in terms of speed, selectivity and resolution of the sample components.

	COMPOUND	ION 300	ORH 801	COREGEL 64H	COREGEL 107H	COREGEL 87H3
1	Malic	12.0	7.5	11.5	10.2	10.0
2	Malonic	11.1	7.4	10.8	9.8	9.8
3	cis-Aconitic	7.5	7.4	11.2	9.9	9.6
4	Adipic	21.8	13.7	21.9	17.5	16.5
5	Formic	17.1	11.1	16.5	15.0	14.6
6	Maleic	8.1	5.2	7.7	7.6	7.8
7	Ascorbic	7.8	5.0	7.5	7.4	10.5
8	Butyric	—	18.5	—	24.1	—
9	Glycolic	15.4	9.9	14.8	13.4	12.8
10	Glycolic	11.5	7.4	11.1	10.1	9.8
12	Citric	9.5	6.3	9.1	8.4	8.3
13	Tartaric	10.0	6.4	9.6	8.9	8.7
14	Nicotinic	—	—	—	—	26.4
15	Propionic	20.1	15.2	21.7	19.3	18.6
16	Succinic	9.2	9.8	8.8	12.7	8.7
18	Oxalic	6.6	4.5	6.5	6.7	6.9
19	Sorbic	18.7	12.0	17.9	16.0	15.3
23	Acrylic	23.3	—	22.5	19.9	19.4
26	Isobutyric	—	—	—	21.8	21.4
27	Lactic	16.0	10.3	15.5	13.6	13.1
28	Shikimic	15.5	9.7	14.7	12.5	12.1
29	Fumaric	16.4	10.3	15.7	14.0	13.1
30	Glutaric	18.2	11.3	17.2	14.7	14.0
31	Pyruvic	9.3	6.0	9.0	8.6	8.7
32	Acetic	—	12.4	18.4	16.6	—
33	Propional	28.7	28.9	—	—	—
36	Quinic	12.6	7.9	12.1	10.7	10.4

Test Conditions: 2.5 mM H₂SO₄, 50 °C, Flow Rate 0.5 mL/minute, 100 ppm

The chart below illustrates the variety of columns available from Concise Separations compared to similar columns offered by other companies:

CONCISE SEPARATIONS	6% XL	6.4% XL	7% XL	8% XL	10% XL	PARTICLE SIZE (µM)
Coregel ARH 601	X					6.5
Coregel 107H					X	8
Coregel 64H		X				10
Coregel 87H1				X		9
Coregel 87H3				X		9
Coregel ION 300	X					7
Coregel ION 310				X		8
Coregel ORH 801			X			9
Coregel USP L17				X		8
Coregel WA1				X		9
Bio-Rad						
Fast Analysis Column				X		9
Fermentation Monitoring				X		9
Aminex™ HPX-87H				X		9
Phenomenex						
Rezex™ RFQ-Fast Acid				X		8
Rezex™ RHM-Monosaccharide				X		8
Rezex™ ROA-Organic Acid				X		8
Shodex						
KC811				N/A		6
Sugar SH1011				N/A		6
Sugar SH1821				N/A		6
Supelco						
SUPELCOGEL™ HPN 59304-U				N/A		9
SUPELCOGEL™ 6-10H				N/A		9
SUPELCOGEL™ HPN 59346				N/A		9


Bio Fuel Analysis

Concise Separations has worked with many Bio Fuel companies to develop Organic Acids columns that better fit their needs. The **107H FA** and the **801 FA** are the latest columns developed out of necessity to stream line important QC steps before and after fermentation.

Coregel 107H FA

PN: ICE-99-9867

The **107H** polymer is unique to Concise Separations. The resolving power coupled with ruggedness allows the polymer to separate organic acids, aldehydes and alcohols in extreme environments. We created the **107H FA** for those Bio Fuel assays that need quick, Reliable results. Ethanol elutes near 7 minutes on the **107H FA** compared to 20 minutes on the original **107H** column.

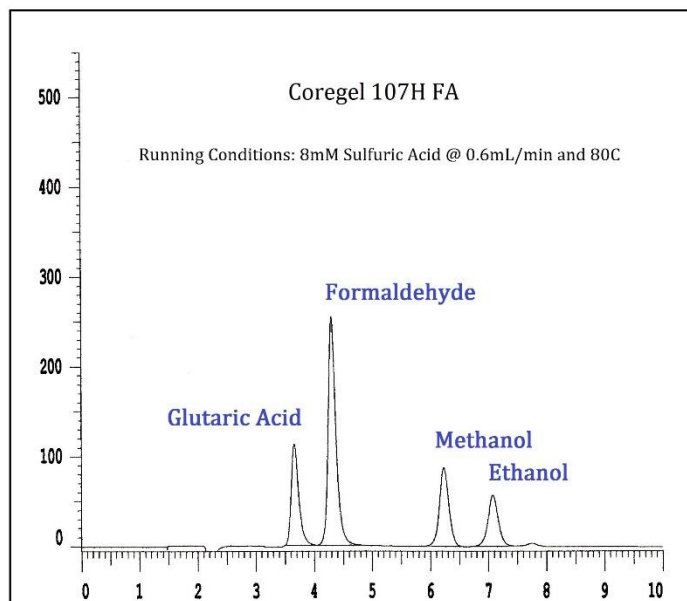


Bio Fuel Analysis

Concise Separations developed another unique column targeted to more complicated Bio Fuel Analysis.

Coregel 801FA


PN: ICE-99-9753

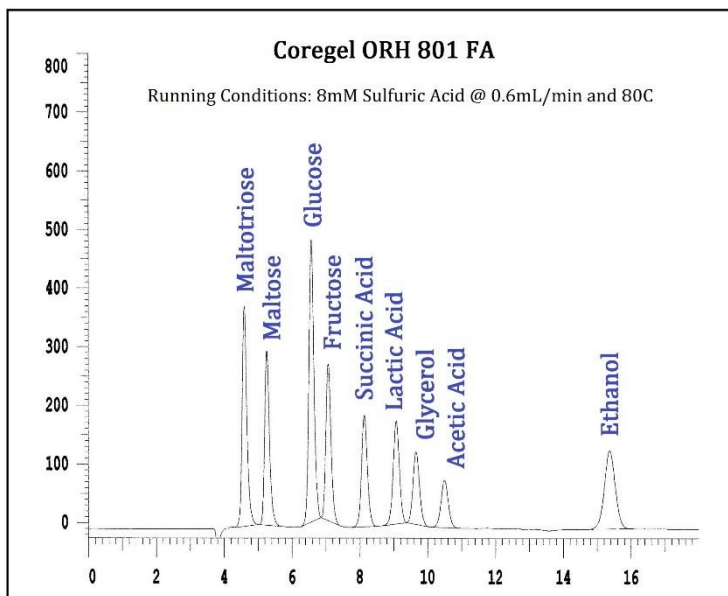

The **801FA** results are much faster than the traditional **ORH 801** column yet peak efficiencies are not compromised.

Organic Acids with Mass Spectrometry

Trifluoroacetic Acid is shown to replace Sulfuric Acid as the eluent. This more volatile acid is favorable for MS Detection.

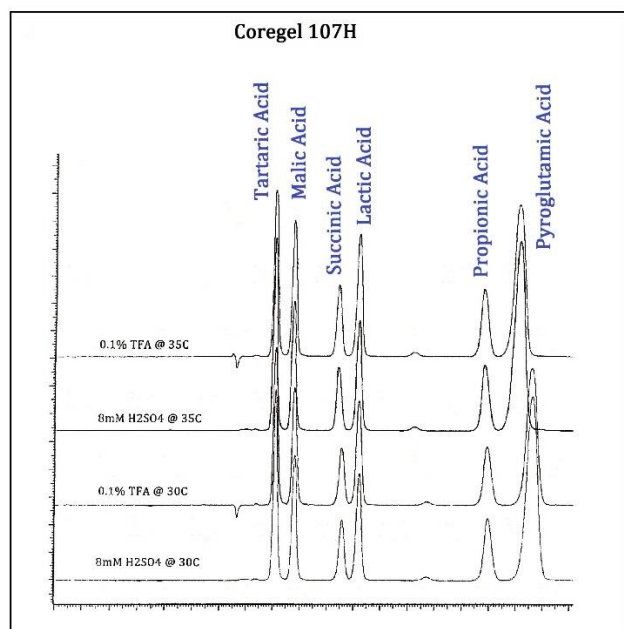


Fermentation Analysis

Concise Separations offers a variety of columns to best fit your fermentation analysis needs. The most popular is shown below.

Coregel 87H3

PN: ICE-99-9861

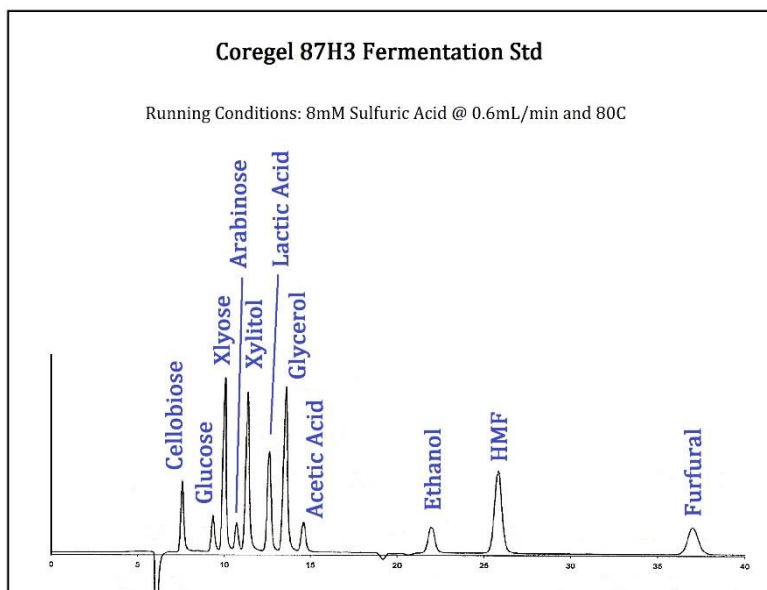


Organic Acid Analysis with Conductivity

Have Conductivity Detector instead of UV? No worries. Concise Separations has a powerful column for you.

Coregel CA1 Carbonate Analysis Column

PN: ICE-99-9872

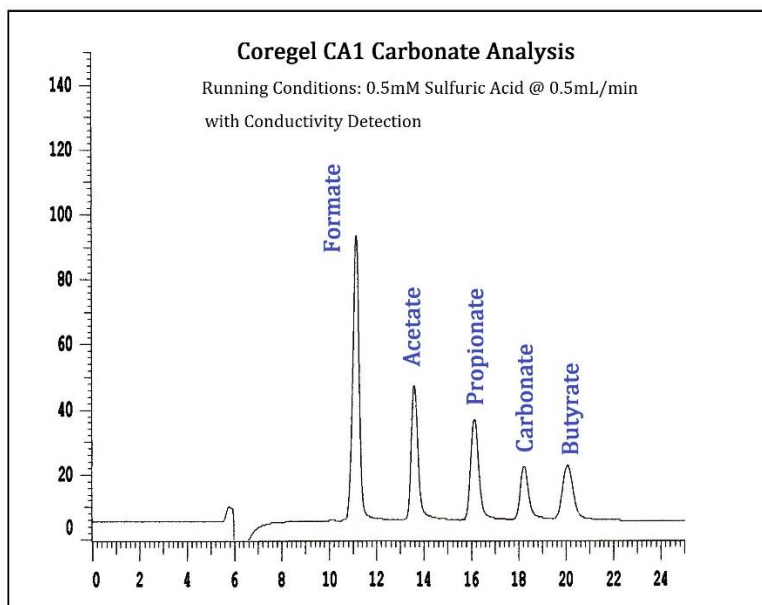

Tips on Maintaining the Performance of Coregel Columns

The most important fact to remember when using Coregel columns is that the polystyrene divinylbenzene copolymer is a low cross-linked material. This polymeric packing has a limited resistance to flow rate and pressure, and will irreversibly compact and overpressure at a certain level. Unlike polymers, silica based materials are not flow rate sensitive and the relation between pressure and flow rate remains relatively constant. Therefore, the Coregel columns should be carefully monitored for pressure, and should be operated within the recommended flow rates and pressure specifications.

- Use column ovens to serve the dual purpose of increasing column efficiency and lowering column back pressure.
- Set the pressure shut off for the analytical test system at or slightly below the recommended pressure maximum for the column to prevent irreversible damage to the column.
- When installing, allow the column to warm up in the column oven for 15 minutes, and then start the flow rate below your target flow rate. After 15 minutes, increase the flow rate to the target flow rate and confirm that the column is operating at the expected back pressure.
- To increase the lifetime of your analytical column, we recommend the proper use of guard columns or cartridges. How frequently you change your guard column depends on pretreatment of the sample.
- Filter and remove potentially harmful organics from the samples to decrease the need to change guard columns. Carefully monitor the guard columns for pressure increase and the chromatograms for changes in retention and efficiency to determine the approximate useful lifetime of the guard columns.


Customer Support

Please do not hesitate to contact us with any question about our products, or help with your application needs. By collaborating with customers to solve new sample separations, we not only provide solutions to problems for our valued customers, we discover new column methods and technologies that can benefit others in our industry. We encourage you to visit our website periodically for updates on new products and applications. We are continuously upgrading the website to provide easier access to specific applications and increase our valuable support information. Please feel free to contact us for website suggestions. Your opinion matters!

Email us: CustomerService@ConciseSeparations.com

Call us: 800-326-2685

Visit us: www.ConciseSeparations.com

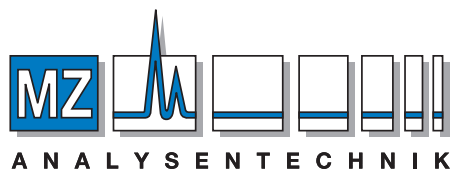

AUTHORIZED DISTRIBUTOR

MZ-Analysentechnik GmbH, Barcelona-Allee 17 • D-55129 Mainz

Tel +49 6131 880 96-0, Fax +49 6131 880 96-20

e-mail: info@mz-at.de, www.mz-at.de



2032 Concourse Dr.
San Jose, CA 95131 USA
800-326-2685

© 2017 Concise Separations. All rights reserved. All other trademarks are the property of their respective owners. For research only. Not for use in diagnostic procedures. Concise Separations is a Division of Edge BioSystems, Inc.

ISO 9001:2008 Certified

**30+ Years of World Class Polymer HPLC
Manufacturing and Innovation**