


# InertSearch for GC

InertCap Applications

## Analysis of Organic acids and Free fatty acids

Data No. GA349-0812

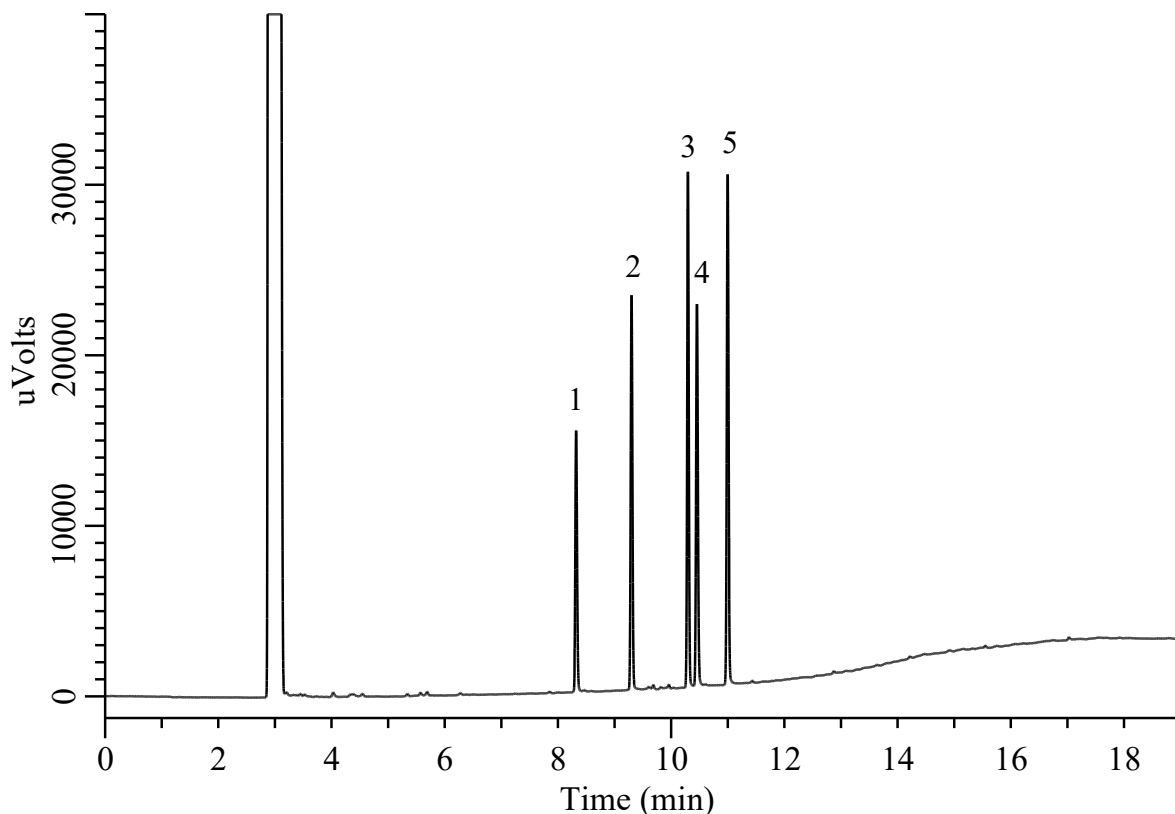


### Conditions

**System** : GC-4000 Plus/FID  
**Column** : InertCap FFAP (GL Sciences Inc.)  
0.25 mm I.D. x 30 m df = 0.25  $\mu$  m  
**Col. Cat. No.** : 1010-28642  
**Col. Temp.** : 80 °C (1 min) - 12 °C/min - 240 °C (5 min)  
**Carrier Gas** : N<sub>2</sub> 65 kPa (0.68 mL/min) , Constant Press.  
**Injection** : Split 1:15  
250 °C  
**Detection** : FID Auto Range  
250 °C  
**Sample Size** : 1  $\mu$  L

### Analyte:

1. Acetic acid
2. Propionic acid
3. Butyric acid
4. Acrylic acid
5. Methacrylic acid

100 ppm(v/v) each



### AUTHORIZED DISTRIBUTOR

MZ-Analysentechnik GmbH, Barcelona-Allee 17 • D-55129 Mainz  
Tel +49 6131 880 96-0, Fax +49 6131 880 96-20  
e-mail: info@mz-at.de, www.mz-at.de

**GL Sciences**