

# InertSearch™ for LC


Inertsil® Applications

## Analysis of Vitamin C (Inertsil NH2)

Data No. LA631-0696


### Analyte:

1. Erythorbic acid (5 mg/L)
2. Ascorbic acid (5 mg/L)

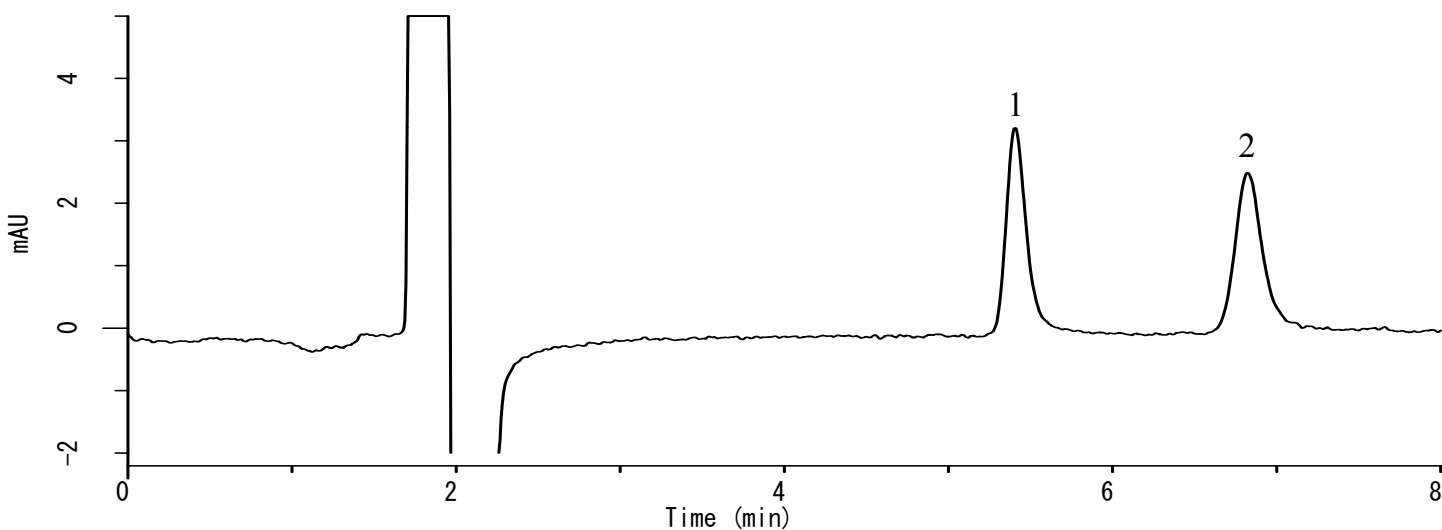

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil NH2 (5 µm, 250 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-05546  
**Eluent** : A) CH<sub>3</sub>CN  
          B) H<sub>2</sub>O  
          C) CH<sub>3</sub>COOH  
          A/B/C = 87/11/2, v/v/v  
**Flow rate** : 2.0 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 243 nm (GL-7452A PDA Detector)  
**Injection Vol.** : 20 µL  
**Sample** : Vitamin C

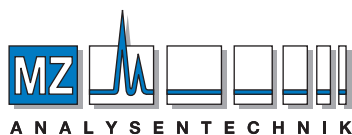


### AUTHORIZED DISTRIBUTOR


MZ-Analysentechnik GmbH, Barcelona-Allee 17 • D-55129 Mainz  
Tel +49 6131 880 96-0, Fax +49 6131 880 96-20  
e-mail: info@mz-at.de, www.mz-at.de

## Analysis of Vitamin C (Inertsil NH2)

Data No. LAxxx-0696

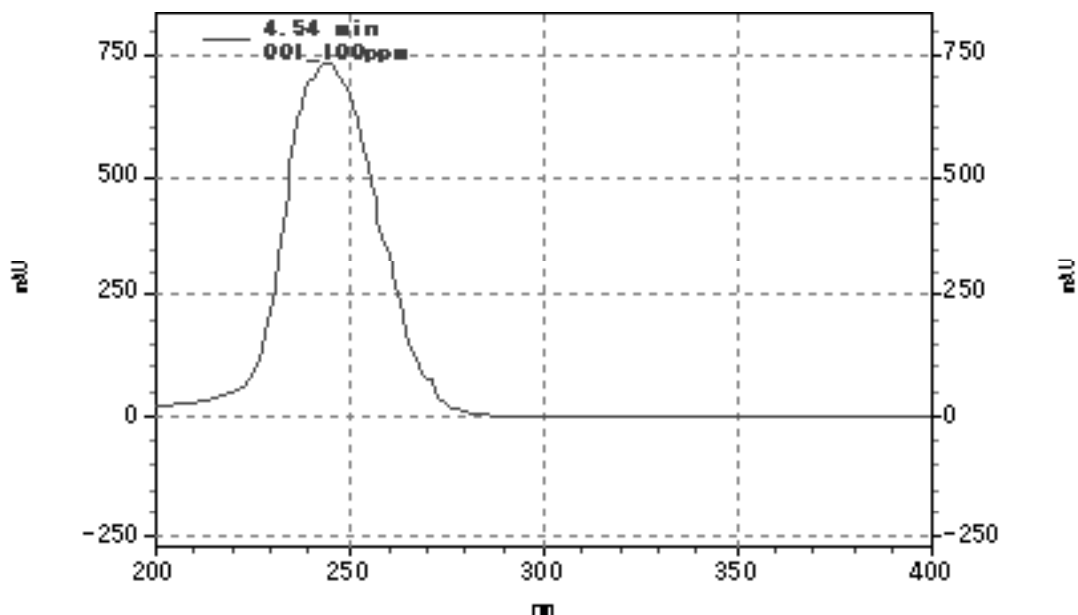

UV spectrum of Erythorbic acid (ErA)

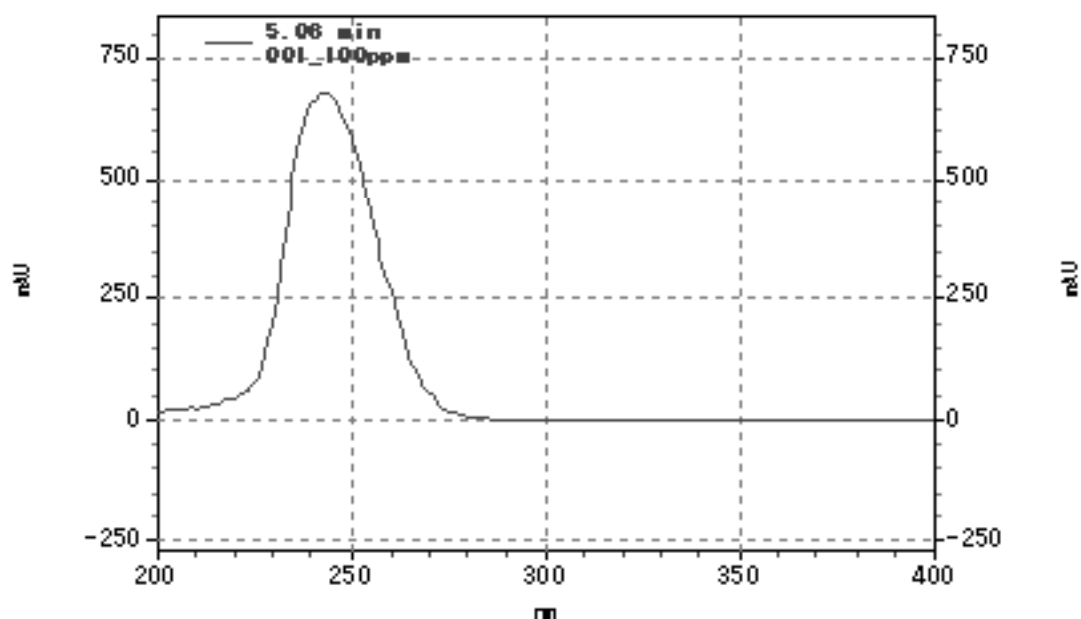

UV spectrum of Ascorbic acid (AsA)