




**GL Sciences' Newest and Most Advanced ODS Phase-New For 2009**

# **Inertsil® ODS-4**

**State-of-the-art C18 HPLC Columns**



Improved Peak Shapes and Heights  
Enhancing Sensitivity  
High Resolution  
Fast Equilibration  
Compatible with 100% Aqueous Eluents

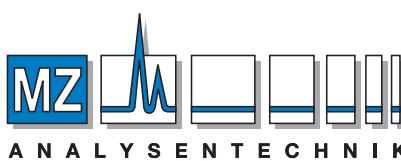

AUTHORIZED DISTRIBUTOR

MZ-Analysentechnik GmbH  
Barcelona-Allee 17 • D-55129 Mainz  
Tel +49 6131 880 96-0  
Fax +49 6131 880 96-20  
e-mail: [info@mz-at.de](mailto:info@mz-at.de)  
[www.mz-at.de](http://www.mz-at.de)

**Ultimate deactivation techniques enabling the highest inertness with the silica base HPLC column allow analyses of trace amount of most demanding basic and acidic compounds.**

**Enhanced deactivation has made the column feature much easier to use!**

# Inertsil® ODS-4

## Enhancing Sensitivity and High Separation Efficiency

Strictly classified particle size with narrow distribution width and ideally designed carbon loading and its procedure allow us to guarantee the high plate count of +100,000/m. Combined with synergistic effect from the improved peak shapes based on the highest inertness of packing material, Inertsil ODS-4 can be used as a tool for enhancing sensitivity and high separation efficiency.



### Excellent peak shapes for both strong acidic and basic compounds

Our newly-developed endcapping technique ideally deactivates the silanol groups, suppressing the adsorption of common basic compounds as well as strong ones, which leads to sharper peaks.

Moreover, the new endcapping technique prevents the adsorption of strong acidic compounds as a surface of the packing material becomes neutral.



### Excellent analysis stability of strong metal chelating compounds

In order to stably analyze strong metal chelating compounds, samples were injected repeatedly before the analysis to mask the adsorption active sites on the surface of the packing material or addition of EDTA to the eluent were required. Column equilibration was also time-consuming. Since the trace amount of metals has been eliminated from the surface of the packing material, it allows a stable analysis from the 1st injection requiring no masking process.



### Excellent analysis stability under 100% aqueous eluents

Inertsil ODS-4 minimizes the dewetting phenomenon while maintaining the same retention characteristics to that of common ODS columns. Therefore, Inertsil ODS-4 can be used at ease under 100% aqueous eluents. Furthermore, the packing material that achieves a stable analysis using 100% aqueous eluents provides another advantage: which reduces the column equilibration time returning to an initial eluent condition in gradient.

## Bonded Phase Structure

–C<sub>18</sub>H<sub>37</sub>


Silica gel	: Highly-pure spherical silica gel	Pore volume	: 1.05 mL/g
Purity	: 99.999%	Bonded phase	: Octadecyl group
Particle size	: 3 µm, 5 µm	Endcapped	: Yes
Surface area	: 450 m <sup>2</sup> /g	Carbon loading	: 11%
Pore size	: 100 Å (10 nm)	USP Code	: L1




## Comparison of inertness to Dextromethorphan between Inertsil® ODS-4 and commercially available ODS columns

Dextromethorphan, a strong basic compound, can be adsorbed by trace amount of residual silanols on the surface of the packing material, resulting in poor peak shapes with the traditional endcapping technique.


Due to its newly-developed powerful deactivation, adsorption of compounds are much less and thus enables highly qualitative analysis of strong basic compounds.

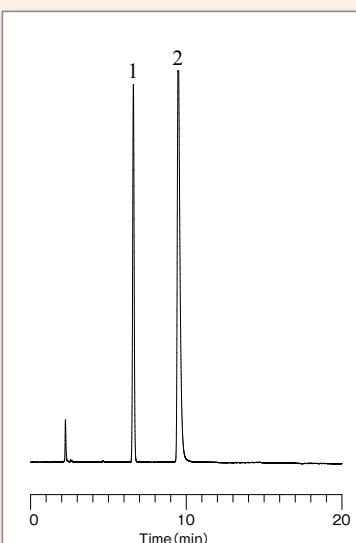


**Inertsil® ODS-4**

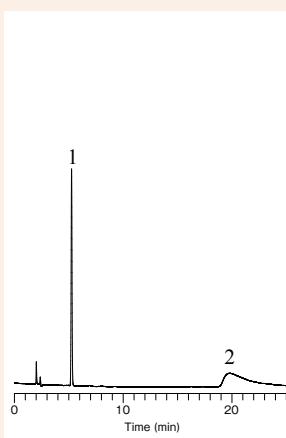


**Symmetry® C<sub>18</sub>**

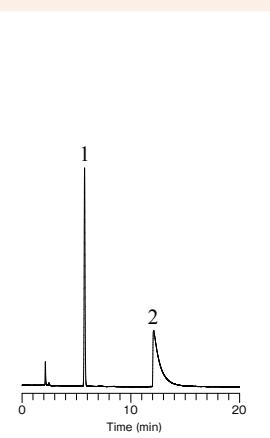


**SunFire™ C<sub>18</sub>**

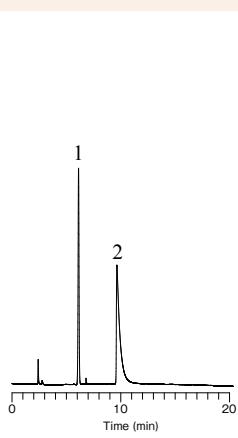


**Atlantis® T3**



**Luna® C<sub>18</sub> (2)**




**ZORBAX Eclipse Plus C<sub>18</sub>**



**Hypersil™ GOLD**

## Analysis of Antihistamines by LC/MS/MS

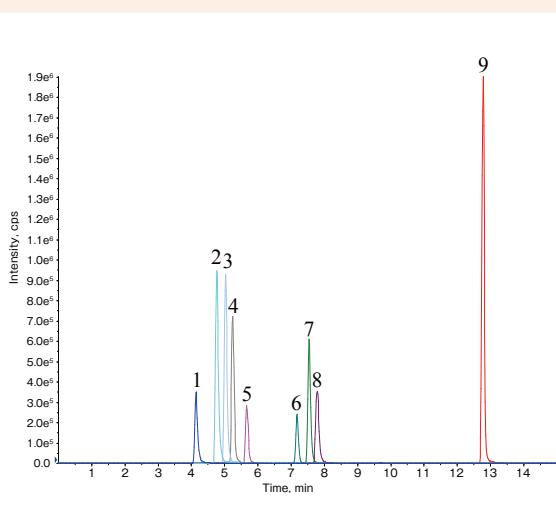

Antihistamines are strongly basic and therefore will easily be adsorbed to the residual silanols on the packing material, resulting in deterioration of peak shapes. Generally, in HPLC analysis of strong basic compounds, highly-concentrated buffer or ion-pair reagents are introduced to the eluent to prevent adsorption of strong basic samples on the packing material. However, in LC/MS (/MS), such eluent conditions are not recommended and a packing material with superb inertness is required.

Inertsil ODS-4 prevents the adsorption of strong basic compounds without using the above mentioned eluents. This feature also makes Inertsil ODS-4 an ideal column for LC/MS (/MS) as well.


Sample:	System
1. Chlorpheniramine (0.1 mg/L)	: LC800 HPLC system 4000 Q TRAP®
2. Cinnarizine (0.1 mg/L)	Column : Inertsil ODS-4 (3 $\mu$ m, 150 $\times$ 2.1 mm I.D.)
3. Clemastine (0.1 mg/L)	Eluent : A) CH <sub>3</sub> OH
4. Difenidol (0.1 mg/L)	B) 2 mM CH <sub>3</sub> COONH <sub>4</sub>
5. Diphenhydramine (0.1 mg/L)	A/B = 40/60 - 10 min- 95/5 - 5 min - 95/5
6. Diphenylpyraline (0.1 mg/L)	Flow Rate : 0.2 mL/min
7. Hydroxyzine (0.1 mg/L)	Col. Temp. : 40 °C
8. Promethazine (0.1 mg/L)	Detection : LC/MS/MS (ESI, Positive, MRM)
9. Triprolidine (0.1 mg/L)	Injection Vol. : 10 $\mu$ L

# Inertsil® ODS-4





## Comparison of inertness to Brilliant Blue FCF between Inertsil® ODS-4 and commercially available ODS columns

Brilliant Blue FCF, a strong acidic compound, will easily be absorbed if the surface of the packing material shows slightly basic. Symmetry C<sub>18</sub>, SunFire C<sub>18</sub>, and Atlantis T3 shown in the figures below, which completely elute weak acids, still have compounds remain uneluted and produce poor peak shapes, due to the adsorption to the packing material. Inertsil ODS-4, as the surface of the packing material is neutral, does not adsorb even strong acid and produce good peak shapes.

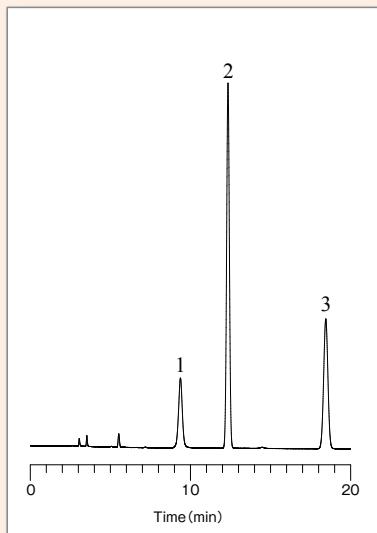


### Inertsil® ODS-4


System	: GL-7400 HPLC system
Column	: 5 $\mu$ m, 250 $\times$ 4.6 mm I.D.
Eluent	: A) CH <sub>3</sub> CN B) 0.1% H <sub>3</sub> PO <sub>4</sub> A/B = 25/75, v/v
Flow Rate	: 1.0 mL/min
Col. Temp.	: 40 °C
Detection	: UV 254 nm
Injection Vol.	: 3.0 $\mu$ L
Sample	: 1. Brilliant Blue FCF (0.05 mg/mL) 2. Phenol (0.3 mg/mL) 3. Salicylic acid (0.2 mg/mL)

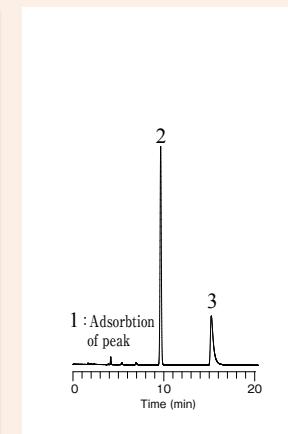


Symmetry® C<sub>18</sub>

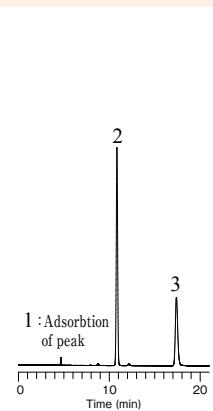


SunFire™ C<sub>18</sub>

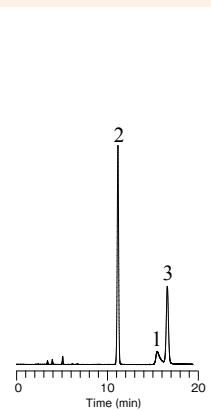


Atlantis® T3

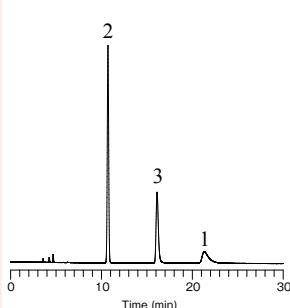

Luna® C18 (2)

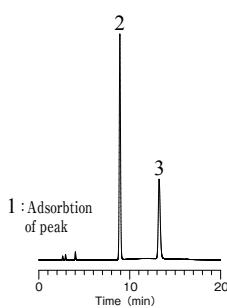


ZORBAX Eclipse Plus C18

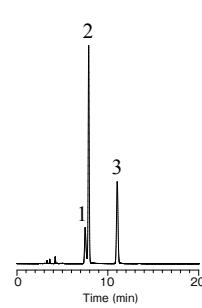

Hypersil GOLD™


## Analysis of Haloacetic Acids by LC/MS/MS

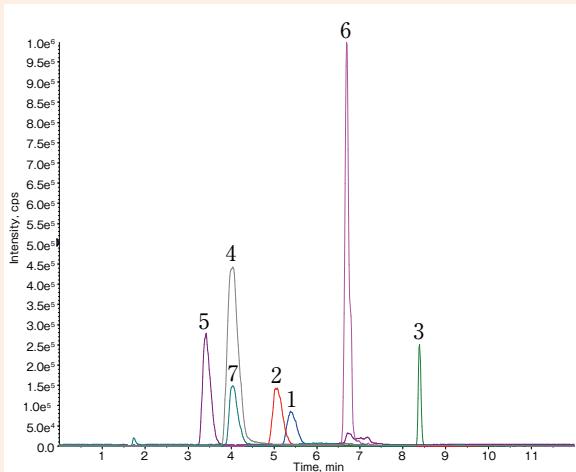

Haloacetic acid is a harmful substance generated when tap water is chlorinated. With its strong acidity, it is easily adsorbed at basic sites on the surface of the packing material. High-sensitivity analysis by LC/MS (/MS) have received attention in these years. In accordance with the popularity, a column free of adsorption has been greatly required since the adsorption of even a very small amount can adversely affect the precision of such highly sensitive quantitative analyses.


Inertsil ODS-4, featuring a neutral packing material surface, is also ideal for LC/MS (/MS) analyses of strong acids.

Sample:	System	: LC800 HPLC system
1. Bromoacetic acid	Column	: Inertsil ODS-4 (3 $\mu$ m, 150 $\times$ 2.1 mm I.D.)
2. Dibromoacetic acid	Eluent	: A) CH <sub>3</sub> OH
3. Tribromoacetic acid		B) 0.1% HCOOH
4. Chloroacetic acid	Flow Rate	A/B = 5/95 - 2.5 min- 5/95 - 2.5 min - 95/5 - 5 min- 95/5
5. Dichloroacetic acid	Col. Temp.	: 40 °C
6. Trichloroacetic acid	Detection	: LC/MS/MS (ESI, Negative, MRM)
7. Bromochloroacetic acid	Injection Vol.	: 10 $\mu$ L




## Comparison of inertness to Hinokitiol between Inertsil® ODS-4 and commercially available ODS columns

Hinokitiol having very strong chelating characteristics, is easily adsorbed with trace metal remaining on a packing material surface. SunFire C<sub>18</sub> in the figure below tend to show a better peak shape every time a new injection is provided, since each new injection covers up more of the adsorption active sites. Inertsil ODS-4 provides very quantitative peaks from the 1st injection since it has completely removed metals from the surface of the packing material.

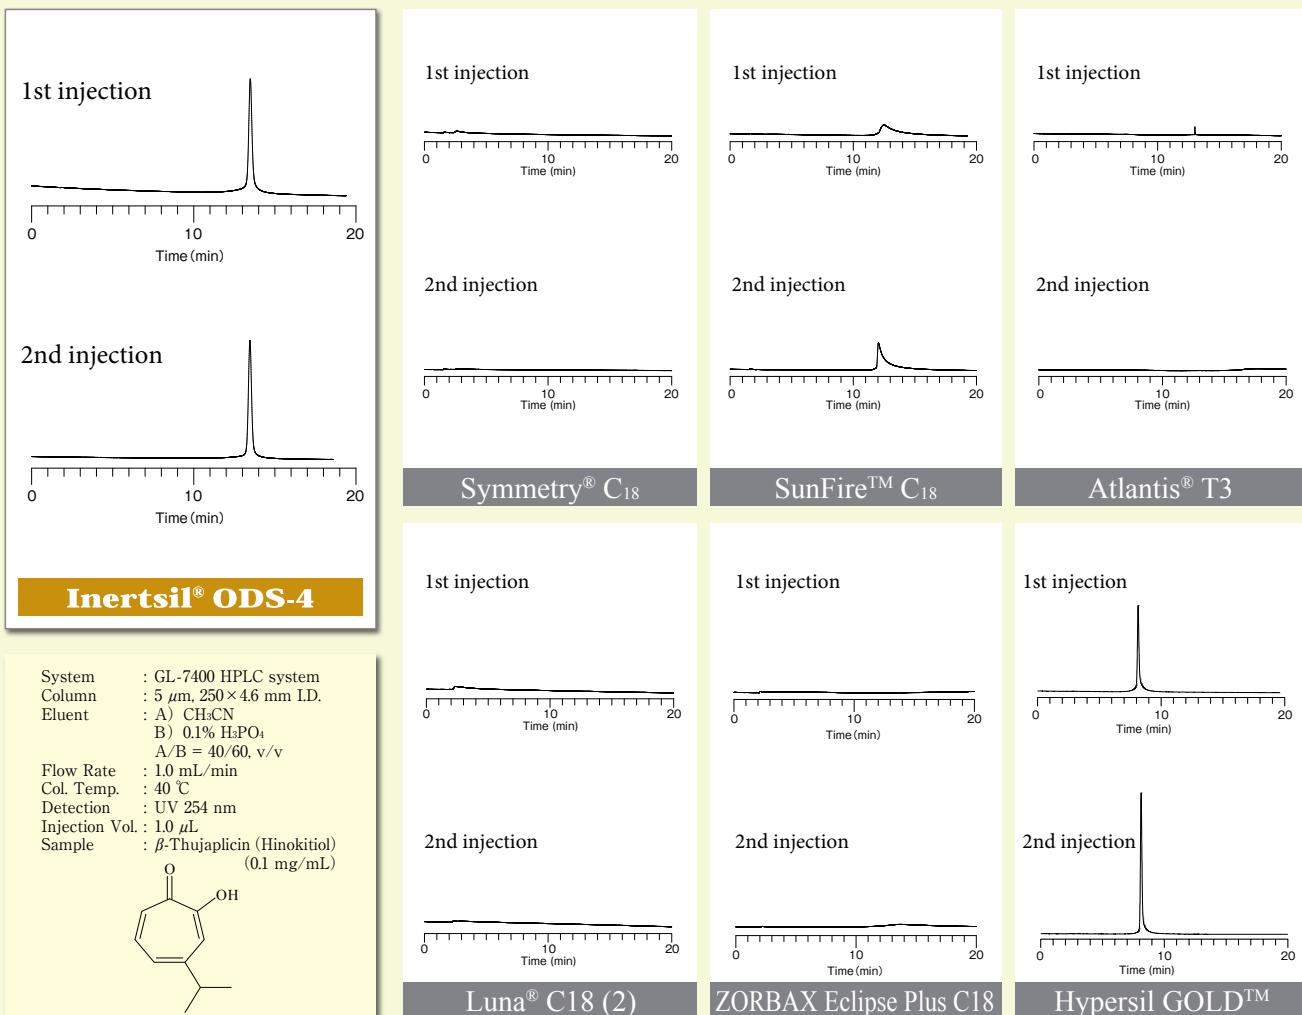

## Analysis of Tetracyclines by LC/MS/MS

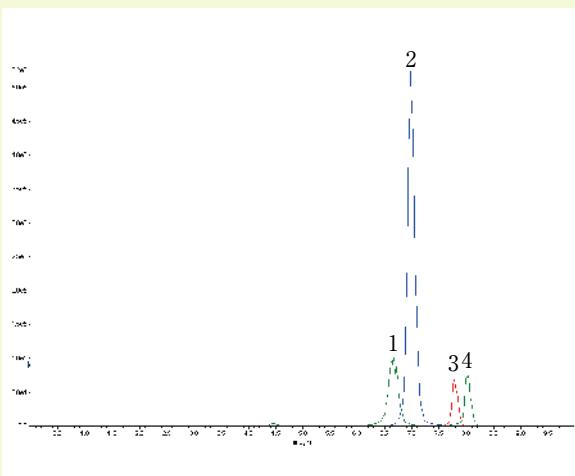

Tetracyclines are antibiotics broadly used as pharmaceuticals for animals, and the residues in livestock and sea product are a major issue today. High-sensitivity analysis by LC/MS ( /MS) has received attention in these years. As tetracyclines have a very strong chelating characteristics, it has been anticipated that the adsorption on the column deteriorates quantitative precision.

Inertsil ODS-4 is an ideal column for LC/MS ( /MS) analyses of chelating compounds as well since it has completely removed metals from the surface of the packing material.


<b>System</b>	: LC800 HPLC system 4000 Q TRAP®
<b>Column</b>	: Inertsil ODS-4 (3 $\mu$ m, 75 $\times$ 2.1 mm I.D. )
<b>Eluent</b>	: A) 0.1% CH <sub>3</sub> OH B) 0.1% HCOOH A/B = 20/80 - 4.5 min- 20/80 - 2 min - 95/5 - 3.5 min- 95/5
<b>Flow Rate</b>	: 0.2 mL/min
<b>Col. Temp.</b>	: 40 °C
<b>Detection</b>	: LC/MS/MS (ESI, Positive, MRM)
<b>Injection Vol.</b>	: 10 $\mu$ L
<b>Sample</b>	: 1. Tetracycline (TC) (100 $\mu$ g/L) 2. Oxytetracycline (OTC) (100 $\mu$ g/L) 3. Chlorotetracycline (CTC) (100 $\mu$ g/L) 4. Doxycycline (DC) (100 $\mu$ g/L)

# Inertsil® ODS-4



## Comparison of analyses under 100% Aqueous Eluents

Under the condition of mobile phase containing very little organic solvent, mobile phase can easily come out from pores in the packing material, resulting in the dewetting phenomenon. As shown in the figures below, such water repellency makes the analysis results unstable over the retention time. Inertsil ODS-4, with an ideal chemical processing, minimizes such dewetting phenomenon, achieving very trustable elution with 100% aqueous eluents.

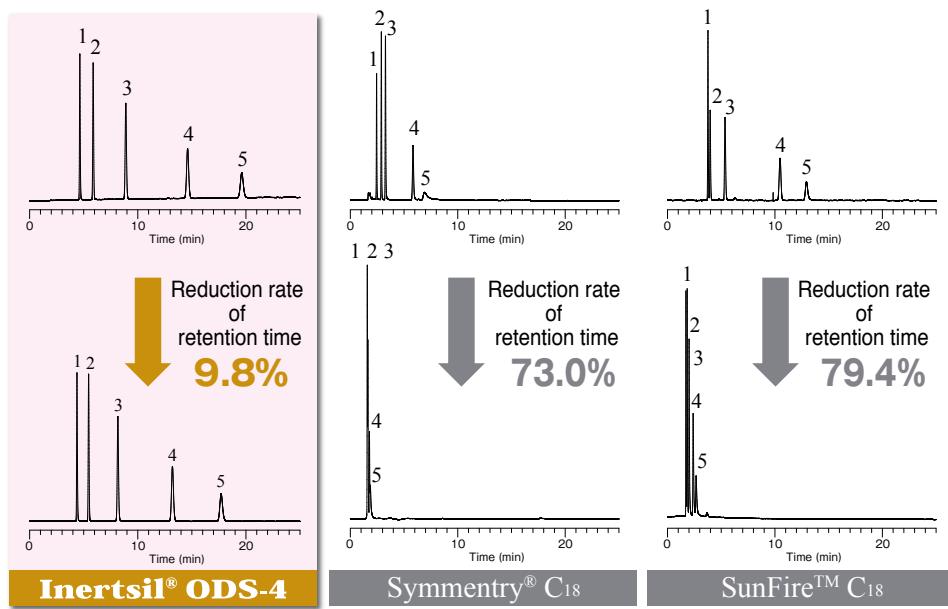

### Testing procedure

- ```

    Introduce 100% water for
    20 minutes.
    ↓
    Analysis (upper chromatograms)
    ↓
    Stop flow for 15 minutes.
    ↓
    Introduce eluent for 30 minutes.
    ↓
    Stop flow for 15 minutes.
    ↓
    Introduce eluent for 15 minutes.
    ↓
    Analysis (lower chromatograms)
  
```

System : GL-7400 HPLC system  
 Column : 5 μm, 250×4.6 mm I.D.  
 Eluent : H<sub>2</sub>O  
 Flow Rate : 1.0 mL/min  
 Col. Temp. : 40 °C  
 Detection : UV 254 nm  
 Sample : 1. Cytosine  
         2. Uracil  
         3. Guanine  
         4. Thymine  
         5. Adenine

## Analytical Column Ordering Information

| Particle size | Diameter (mm) | 1.0        | 1.5        | 1.0 ~ 1.5 | 2.1        | 3.0        | 4.0        | 4.6        | 2.1 ~ 4.6 |
|---------------|---------------|------------|------------|-----------|------------|------------|------------|------------|-----------|
|               | Length (mm)   | Cat.No.    | Cat.No.    | Price     | Cat.No.    | Cat.No.    | Cat.No.    | Cat.No.    | Price     |
| 3 μm          | 30            | 5020-81111 | 5020-81121 |           | 5020-04011 | 5020-04021 | 5020-04031 | 5020-04041 |           |
|               | 50            | 5020-81112 | 5020-81122 |           | 5020-04012 | 5020-04022 | 5020-04032 | 5020-04042 |           |
|               | 75            | 5020-81113 | 5020-81123 |           | 5020-04013 | 5020-04023 | 5020-04033 | 5020-04043 |           |
|               | 100           | 5020-81114 | 5020-81124 |           | 5020-04014 | 5020-04024 | 5020-04034 | 5020-04044 |           |
|               | 150           | 5020-81115 | 5020-81125 |           | 5020-04015 | 5020-04025 | 5020-04035 | 5020-04045 |           |
|               | 250           | 5020-81116 | 5020-81126 |           | 5020-04016 | 5020-04026 | 5020-04036 | 5020-04046 |           |
| 5 μm          | 30            | 5020-81011 | 5020-81021 |           | 5020-03911 | 5020-03921 | 5020-03931 | 5020-03941 |           |
|               | 50            | 5020-81012 | 5020-81022 |           | 5020-03912 | 5020-03922 | 5020-03932 | 5020-03942 |           |
|               | 75            | 5020-81013 | 5020-81023 |           | 5020-03913 | 5020-03923 | 5020-03933 | 5020-03943 |           |
|               | 100           | 5020-81014 | 5020-81024 |           | 5020-03914 | 5020-03924 | 5020-03934 | 5020-03944 |           |
|               | 150           | 5020-81015 | 5020-81025 |           | 5020-03915 | 5020-03925 | 5020-03935 | 5020-03945 |           |
|               | 250           | 5020-81016 | 5020-81026 |           | 5020-03916 | 5020-03926 | 5020-03936 | 5020-03946 |           |

\* The joint is Waters 1/16" type. \* For other column sizes, please contact us.

## Preparative Column Ordering Information

| Diameter (mm) | 6.0        |       | 7.6        |       | 10.0       |       | 20.0       |       |
|---------------|------------|-------|------------|-------|------------|-------|------------|-------|
| Length (mm)   | Cat.No.    | Price | Cat.No.    | Price | Cat.No.    | Price | Cat.No.    | Price |
| Guard 50      | 5020-03957 |       | 5020-03967 |       | 5020-81057 |       | 5020-81067 |       |
| 100           | 5020-03954 |       | 5020-      |       | 5020-      |       | 5020-      |       |
| 150           | 5020-03955 |       | 5020-      |       | 5020-      |       | 5020-      |       |
| 250           | 5020-03956 |       | 5020-03966 |       | 5020-81056 |       | 5020-81066 |       |

\* The joint is Waters 1/16" type. \* For other column sizes, please contact us.

## Cartridge Guard Column Ordering Information

| Diameter of the analytical column applicable (mm) | Diameter of the guard column (mm) | Length of the guard column (mm) | Replacement cartridge guard columns (2/pk) |       | Holder/Cartridge set (1 holder and 2 cartridges) |       |
|---------------------------------------------------|-----------------------------------|---------------------------------|--------------------------------------------|-------|--------------------------------------------------|-------|
|                                                   |                                   |                                 | Cat.No.                                    | Price | Cat.No.                                          | Price |
| 1.0                                               | 1.0                               | 10                              | 5020-08517                                 |       | 5020-08527                                       |       |
| 1.5 , 2.1                                         | 1.5                               | 10                              | 5020-08518                                 |       | 5020-08528                                       |       |
| 2.1 , 3.0                                         | 3.0                               | 10                              | 5020-08515                                 |       | 5020-08525                                       |       |
|                                                   |                                   | 20                              | 5020-08565                                 |       | 5020-08575                                       |       |
| 4.0 , 4.6                                         | 4.0                               | 10                              | 5020-08510                                 |       | 5020-08520                                       |       |
|                                                   |                                   | 20                              | 5020-08560                                 |       | 5020-08570                                       |       |

\* The only joint available is Waters 1/16" type. \* Please specify the packing material and the particle size in your order.


\* We also have other guard column (GL-cart) as well. Please inquire for further details.

## Applications

### Food additives

System : GL-7400 HPLC system  
 Column : Inertsil ODS-4 (5  $\mu$ m, 150  $\times$  4.6 mm I.D.)  
 Eluent : A) CH<sub>3</sub>CN  
 B) 25 mM CH<sub>3</sub>COONa (pH 4.6, CH<sub>3</sub>COOH)  
 A/B = 10/90 - 4 min - 10/90 - 16 min - 40/60 - 10 min - 40/60  
 Flow Rate : 1.0 mL/min  
 Col. Temp. : 40 °C  
 Detection : UV 238 nm  
 Injection Vol. : 10  $\mu$ L  
 Sample : Food additives


|                                          |           |
|------------------------------------------|-----------|
| 1. Sodium Saccharin                      | (50 mg/L) |
| 2. p-Hydroxy benzoic acid                | (50 mg/L) |
| 3. Sorbic acid                           | (50 mg/L) |
| 4. Benzoic acid                          | (50 mg/L) |
| 5. p-Hydroxy benzoic acid methyl ester   | (50 mg/L) |
| 6. Dehydroacetic Acid                    | (50 mg/L) |
| 7. p-Toluid acid                         | (50 mg/L) |
| 8. p-Hydroxy benzoic acid ethyl ester    | (50 mg/L) |
| 9. p-Hydroxy benzoic acid n-propyl ester | (50 mg/L) |

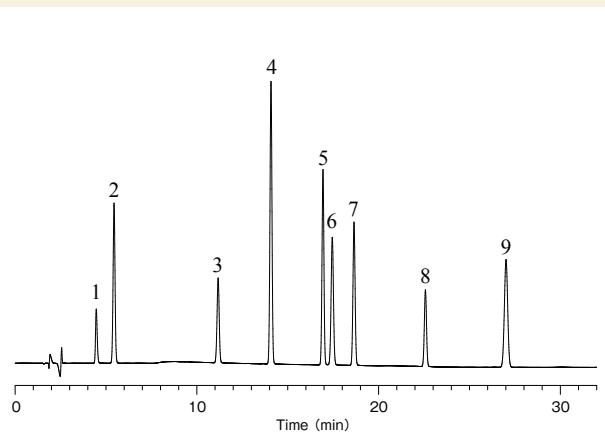

### Nucleic acid bases

System : GL-7400 HPLC system  
 Column : Inertsil ODS-4 (5  $\mu$ m, 150  $\times$  4.6 mm I.D.)  
 Eluent : 0.1M KH<sub>2</sub>PO<sub>4</sub>, 0.2M NaClO<sub>4</sub> (pH 2.0, H<sub>3</sub>PO<sub>4</sub>)  
 Flow Rate : 1.0 mL/min  
 Col. Temp. : 40 °C  
 Detection : UV 254 nm  
 Injection Vol. : 1  $\mu$ L  
 Sample : Nucleobase


|               |           |
|---------------|-----------|
| 1. Cytosine   | (25 mg/L) |
| 2. Uracil     | (25 mg/L) |
| 3. Guanine    | (25 mg/L) |
| 4. Adenine    | (25 mg/L) |
| 5. Cytidine   | (25 mg/L) |
| 6. Uridine    | (25 mg/L) |
| 7. Thymine    | (25 mg/L) |
| 8. Adenosine  | (50 mg/L) |
| 9. Guanosine  | (50 mg/L) |
| 10. Thymidine | (50 mg/L) |

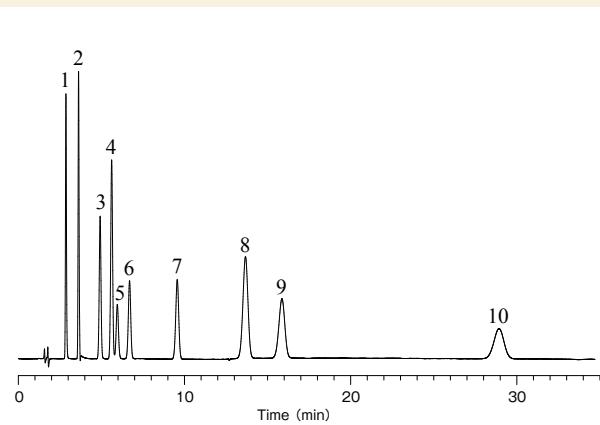

### Efficient ingredients in a cold medicine

System : GL-7400 HPLC system  
 Column : Inertsil ODS-4 (5  $\mu$ m, 150  $\times$  4.6 mm I.D.)  
 Eluent : A) CH<sub>3</sub>CN  
 B) 0.1% H<sub>3</sub>PO<sub>4</sub>  
 A/B = 3/97 - 20 min - 75/25  
 Flow Rate : 1.0 mL/min  
 Col. Temp. : 40 °C  
 Detection : UV 210 nm  
 Injection Vol. : 10  $\mu$ L  
 Sample : Anti-Cold medicine


|                        |           |
|------------------------|-----------|
| 1. Maleic acid         | (50 mg/L) |
| 2. Acetaminophen       | (50 mg/L) |
| 3. Caffein             | (50 mg/L) |
| 4. Chlorpheniramine    | (50 mg/L) |
| 5. Ethenzamide         | (50 mg/L) |
| 6. Bromovalerylurea    | (50 mg/L) |
| 7. Apronalide          | (50 mg/L) |
| 8. Isopropylantipyrine | (50 mg/L) |
| 9. Ibuprofen           | (50 mg/L) |

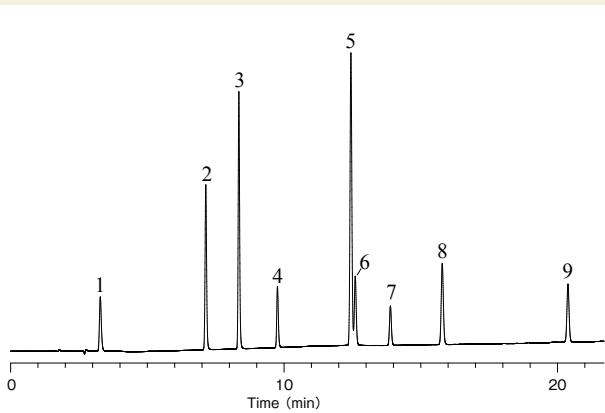

### Tricyclic antidepressant

System : LC800 HPLC system  
 API 3000  
 Column : Inertsil ODS-4 (5  $\mu$ m, 100  $\times$  2.1 mm I.D.)  
 Eluent : A) CH<sub>3</sub>CN  
 B) 10 mM CH<sub>3</sub>COONH<sub>4</sub> (pH 7.0, CH<sub>3</sub>COOH)  
 A/B = 60/40, v/v  
 Flow Rate : 0.2 mL/min  
 Col. Temp. : 40 °C  
 Detection : LC/MS/MS (ESI, Positive, MRM)  
 Injection Vol. : 1  $\mu$ L  
 Sample : Antidepressant agent

|                  |            |
|------------------|------------|
| 1. Imipramine    | (100 mg/L) |
| 2. Clomipramine  | (100 mg/L) |
| 3. Amitriptyline | (100 mg/L) |
| 4. Mianserin     | (100 mg/L) |

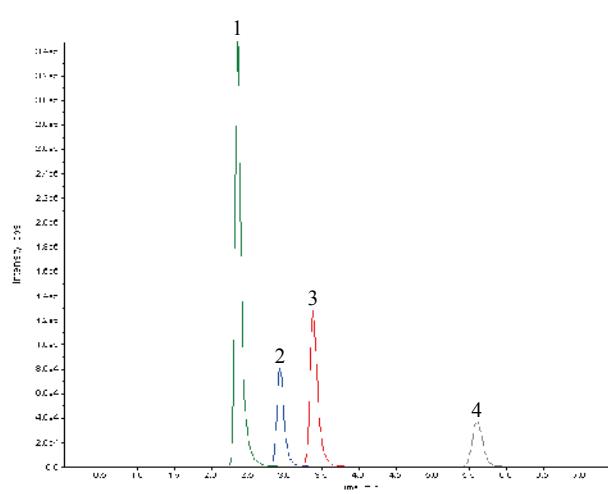

# WORLDWIDE Ordering Information

Inertsil® HPLC columns are available through our authorized distributors in the following countries.



## ■ ARGENTINA

Omnilab Srl.  
Virrey Arredondo 2850  
C1426EAB-Buenos Aires,  
Argentina  
Tel: 11-4553-1100  
Fax: 11-4555-1584



## ■ AUSTRALIA

Winlab Pty Ltd.  
5/2 Pinacle Street Brendale  
Queensland,Australia 4500  
Tel: 07-3205-5233  
Fax: 07-3205-1231



## ■ AUSTRIA

CP Analytik GmbH  
Am Pulverturm 17  
A-2130 Mistelbach  
Tel: 2572-4381  
Fax: 2572-20791



## ■ BELGIUM

Achrom, n.v.s.a  
Philipstraat 5  
9870 Machelen-Zulte  
Tel: 9-380-06-47  
Fax: 9-386-08-86



## ■ BRAZIL

Alpha Center  
rua Senador Fláquer, 877 - conjunto 72  
Casa Branca - Santo André(SP) 09010-160  
Brazil  
Tel: +55(11)2122-0206  
Fax: +55(11)4152-2593

Cromatec Soluções Analíticas  
Rua Charles Darwin, 483  
Vila Sta. Catarina, CEP. 04379-060  
Sao Paulo - SP, Brazil  
Tel: 55 11 5670.2510  
Fax: 55 11 5670.2522



## ■ CANADA

Life Science  
365 Lansdowne Street East  
Peterborough,  
Ontario,K9J 6X9 Canada  
Tel: 705-749-9557  
Fax: 705-749-9139




## ■ CHILE

Genesys Chile Ltda.  
Av.José Domingo Canas 570. Nunoa,  
Santiago, Chile.  
Tel: (562)269-0360  
Fax: (562)269-9597



## ■ CHINA

島津技販(上海)貿易有限公司  
Shimadzu-GL Sciences (Shanghai)  
公司地址:淮海西路570号红坊创业园E幢2楼  
郵編:200052  
電話:(021 ) 628002 (代表)  
傳真:(021 ) 52583319  
http://www.shimadzu-gl.com.cn



## ■ CZECH REPUBLIC

Watrex Praha s.r.o.  
Hostalkova 42 169 00 Praha 6  
Czech Republic  
Tel: 02-220-513-446  
Fax: 02-220-513-448



## ■ DENMARK

Mikrorab Aarhus A/S  
Axel Kiers Vej 34 8270Hojbjerg,  
Denmark  
Tel: 86-29-61-11



## ■ EGYPT

SPECTRA EGYPT  
808 ELBORG ELKEBLY BUILDING  
GIZA SQUARE, EGYPT  
Tel: (202)5721529  
Fax: (202)5729745



## ■ FINLAND

Norlab Oy  
P.O.Box 44  
Vanhanlyntie 12/4 Hameenkylän  
kartano 01721 Vantaa,Finland  
Tel: 09-8545-510  
Fax: 09-8545-5151



## ■ FRANCE

Interchim  
211 bis, avenue JF Kennedy  
BP1140  
03103 Montluçon cedex  
Tel: 04-70-03-88-55  
Fax: 04-70-03-82-60



## ■ GERMANY

MZ AnalyseTechnik GmbH  
Barcelona-Allee 17, D-55129 Mainz, Germany  
Tel: +49 6131 980 96-0  
Fax: +49 6131 880 96-20  
e-mail: info@mz-at.de  
www.mz-at.de



## ■ HONG-KONG

South East Chemicals & Instruments Ltd.  
1210 Chai Wan Industrial City Phase 1,60  
Wing Tai Road Chai Wan. Hong Kong  
Tel: 2802-6333  
Fax: 2807-0542  
Chelleson Scientific Instruments Company  
Units 1210-1212, 12/F., Metro Loft,  
38 Kwai Hei Street, Kwai Chung, N.T., Hong Kong  
Tel: +852 2413 6700  
Fax: +852 2402 4885



## ■ INDIA

LCGC SUPER MARKET  
LCGC Towers, 161/166, Paigah Colony,  
Near Anand Theatre, S.P.Road,  
Secunderabad 500 003  
Tel: 040-66315242/66315243  
Reliance Mobile: 9347015242  
Fax: 040-66329000



## ■ INDONESIA

P.T.Batuwaris Dinamika  
Cahaya Palmerah Building,3Th  
Floor,Room 305 JL.Palmerah Utara 3/9  
Jakarta Barat 11480,Indonesia  
Tel: 021-530-7069  
Fax: 021-530-7069



## ■ IRELAND

Carl Stuart Limited  
Tallaght Business Park, Whitestown,  
Dublin 24 Ireland  
Tel: 01-4523432 / 4523222  
Fax: 01-4523967



## ■ ISRAEL

Ophir Analytical Ltd.  
6. Hamelaha  
P.o.Box 11616 St Park-Afek  
Rosh-Haayn 48091 Israel  
Tel: 972-3902-2277  
Fax: 972-3902-2488



## ■ ITALY

CPS Analytical S.R.L.  
Via Neera 8/A  
20141 Milano - Italy  
Tel: 02 8954201  
Fax: 02 89542022  
Microcolumn S.R.L.  
Via Carlo Porta-20035 Lissone Mi-Italy  
Tel: 039-2143470  
Fax: 039-2143472



## ■ JORDAN

Dijila Est.For Laboratory Consumables.  
P.O.Box 2737 Amman 11953 Jordan  
Tel: 079-5557012



## ■ KOREA

International C.S.  
RM713, WOOLIM E-BIZ CENTER, 170-5  
GURO-DONG GURO-GU, SEOUL, KOREA  
Tel: 02-2108-2350  
Fax: 02-2108-2354



## ■ MALAYSIA

Alpha Analytical (M) Sdn. Bhd.  
No. 47A, Jalan Anggerik Vanilla N31/N  
Kota Kemuning, 40460 Shah Alam  
Selangor Darul Ehsan  
Tel: (603)-5124-6088  
Fax: (603)-5124-6068



## ■ THE NETHERLANDS

ATAS GL International B.V.  
De Sleutel 9  
5652 AS Eindhoven The Netherlands  
Tel: +31(0)40 2549531  
Fax: +31(0)40 2549779  
E-mail: info@atasgl.com  
URL: www.atasgl.com, www.inertsil.nl




## ■ NORWAY

Holger Teknologi as  
Postboks 122 Holmlia  
NO 1202 OSLO  
Telefon: (+47) 23 16 94 60  
Fax: (+47) 22 61 10 30  
E-post: post@holger.no



## ■ PHILIPPINES

Shimadzu Philippines Corporation  
12TH FLOOR 88 CORPORATE CENTER  
141 SEDENO CORNER VALERO STREET,  
SALCEDO VILLAGE, MAKATI CITY, PHILIPPINES  
Tel: (632)889-6219, 889-7252  
Fax: (632)889-7251



## ■ SAUDI-ARABIA

ZALMA for Medical&Laboratory Supplies  
Al-dekheil Center,Office No.56,Falasteen  
Street,Jeddah,Kingdom of Saudi Arabia  
Tel: 2-6655352  
Fax: 2-6655958

## ■ SINGAPORE

ALPHA ANALYTICAL(S)PTE LTD  
71 Toh Guan Road East, #02-01/02 TCH Tech Centre,  
Singapore 608598  
Tel : (65)6567 8885  
Fax: (65)6567 2977  
M : (65)9766 0713  
E-mail: john.wong@alpha-analytical.com.sg  
URL: www.alpha-analytical.com.sg



## ■ SPAIN

Akady  
Calle De Sants 387 5 o 3a  
08028 Barcelona,Spain  
Tel: 93-449-34-51

Teknokroma S.C.C.L.  
08190 Sant Cugat Del Valles,  
Barcelona,Spain  
Tel: 93-674-88-00  
Fax: 93-675-24-05

Sugelabor,S.A.  
Calle Sicilia,36,28038 Madrid,Spain  
Tel: 91-501-39-36  
Fax: 91-501-39-38



## ■ SWEDEN

Scantec Lab AB  
Box 238, S-433 24  
Partille, Sweden  
Tel: 31-336-90-00  
Fax: 31-336-90-36



## ■ SWITZERLAND

BGB Analytik AG  
Rohmattstrasse 4  
4461 Boeckten  
Tel: 61-991-00-46  
Fax: 61-991-00-25



## ■ TAIWAN

Vercotech Inc.  
6F No.7-1 An Hsing Road,  
Hsin Tien,Taipei, Taiwan  
231 R.O.C.  
Tel: 02-2211-3939  
Fax: 02-2211-5522



## ■ THAILAND

Bara Scientific Co.,Ltd.  
Av Chu Liang Building, Floor 7 968 Rama 4  
Road, Bangkok, Bangkok 10500, Thailand  
Tel: 02-6324300  
Fax: 02-6375496-7




## ■ TURKEY

ANT TEKNIK CIHAZLAR PAZ.VE DIS.TIC.LTD.STI  
BURHANIYE MAH.BEYBOSTANI SOK.  
NO:37/1 BEYLBEYI 34676-ISTANBUL TURKEY  
Tel: 90 216 422 67 00  
Fax: 90 216 422 39 54



## ■ UNITED KINGDOM

Hichrom Limited  
1 The Markham Centre, Station  
Road, Theale, Reading, Berkshire, RG7  
4PE, England  
Tel: 0118-930-3660  
Fax: 0118-932-3484



## ■ UNITED STATES

GL Sciences Inc. U.S.A  
4733 Torrance Blvd, Ste 255  
Torrance, CA 90503  
Tel: (310) 265-4424  
Fax: (310) 265-4425  
URL: http://www.inertsil.com



## ■ VIETNAM

2H Instrument  
Collective Quarter of Law  
Tran Quoc Hoan Str, Cau Giay  
Ha Noi, Vietnam  
Tel: +84 4-79-111-79  
Fax: +84 4-79-111-80  
E-Mail: 2hins@hn.vnn.vn



## GL Sciences Inc.

22-1 Nishishinjuku 6-chome  
Shinjuku-ku, Tokyo, 163-1130 Japan  
Phone : +81-3 (5323) 6620  
Fax : +81-3 (5323) 6621  
e-mail : world@gls.co.jp  
URL : http://www.inertsil.com. or  
http://www.gls.co.jp/index\_e.html

Concerning the countries that are not listed above, please contact us directly.