



Vitamin B₆ (1)

The components of vitamin B₆ family resemble each other in structure and are difficult to separate. Usually, the method using ion pair reagent is used. However, under strong acidic conditions such as at pH 2.0, separation is possible by reversed phase mode using the slight difference of hydrophilicity. Three components of vitamin B₆ family were separated with the Asahipak ODP-50 6D column, which can be used even at pH2.0.

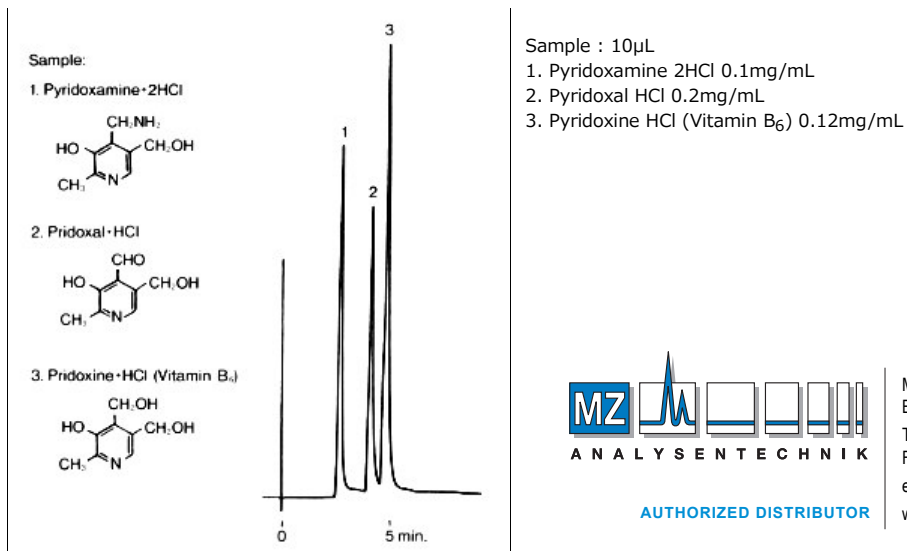

AUTHORIZED DISTRIBUTOR

MZ-Analysentechnik GmbH
Barcelona-Allee 17 • D-55129 Mainz
Tel +49 6131 880 96-0
Fax +49 6131 880 96-20
e-mail: info@mz-at.de
www.mz-at.de

Column : Shodex Asahipak ODP-50 6D (6.0mmI.D. x 150mm)
Eluent : 50mM Sodium Phosphate buffer (pH2.0)
Flow rate : 1.0mL/min
Detector : UV (254nm)
Column temp. : 30°C