


HPLC Separation of Acrylamide and Melamine

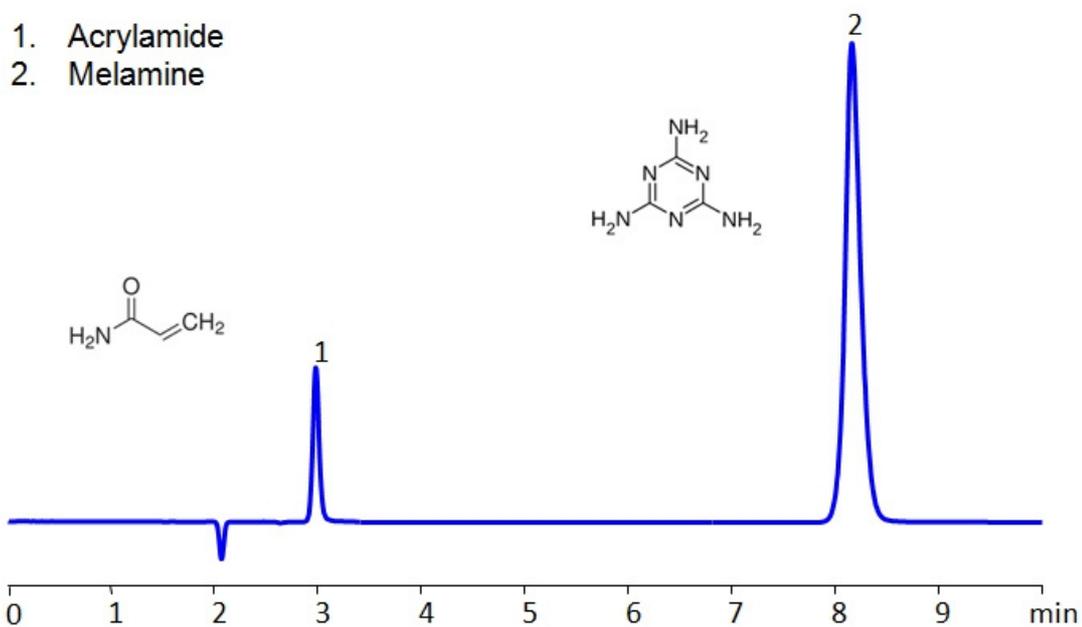

Column:	Primesep 200
Column size:	4.6 × 150 mm, 3 μm
Mobile phase:	H ₂ O - 99%
Buffer:	Formic Acid – 1%
Flow rate:	1 mL/min
UV detection:	240 nm